

Intercomparison of absorption photometer Project: AP-2020-3-3

Location of the quality assurance: TROPOS, Lab 121

Date: 2020-10-23 to 2020-10-30

Principal Investigator	Institution	Participant	Instrument SN
M. Schütze	UBA	M. Schütze	159

Intercomparison summary

Status on arrival

No issues due to transportation or other damages.

Flow calibration

The flow meter of the instrument is set to report flow for conditions of 0 °C and 1013.25 hPa. The deviation of the flow was 0.6% compared to reference flow meter (TSI 4100). Corrections for the flow deviation and the temperature and pressure (STP correction) were considered in the data evaluation.

Instrumental Noise

The noise level of the instrument is out of the normal range. The average noise (1σ) was less equal 71 ng m^{-3} for 5 minute averaging time. The background level was acceptable with deviations of less equal 1 ng m^{-3} .

Inspection

The sensor head was slightly contaminated. The sensor head was cleaned. A flow recalibration was not performed.

Comparison to reference MAAP

BC concentrations of MAAP are 3.9 % higher than BC concentrations from a reference MAAP.

Comparison to reference absorption

BC concentrations of MAAP are 16.2 % higher than BC concentrations from a reference MAAP.

Recommendations

No recommendations.

Overall assessment

The instrument meets the requirements.

Details

Configuration parameters

THERMO SCIENTIFIC	MAAP v1.33	SERIENNUMMER	159	20-10-23
<hr/>				
SIGMA BC:	6.6 m ² /g			
LUFTDURCHSATZ l/h	480			
MITTELWERTSPEICHER:	0 min			
KONZ. BEZOGEN AUF	NORMTEMPERATUR			
NORMTEMPERATUR	0 °C			
DRUCKFORMAT:	COM2	7		
DRUCKZYCLUS:	0 s			
BAUDRATE:	Bd COM1	9600		
BAUDRATE:	Bd COM2	9600		
GERAETE-ADRESSE:	50			
FILTERWECHSEL				
TRANSM. <	%	45		
ZYCLUS	h	100		
UHRZEIT	UHR	24		
SENSORKALIBRIERUNG				
T1	T2	T3	T4	P1 P2 P3
-14	0	-60	68	32 -106 -6
LUFTDURCHSATZ	94.9			
HEIZUNGSPARAMETER				
Sollwert T2 UEBER T1	0 °C			
Max. Heiztemperatur	45 °C			
Min. Heizleistung	10 %			
ANALOGAUSGAENGE				
AUSGABENULLPUNKT:	4mA			
CBC	0 10			
MBC	0 2400			
GESYTEC-PROTOKOLL				
STATUSBELEGUNG	STANDARD			
VARIABLEN-ANZAHL	1			
CBC				
END				

Flow check

Table 2: Correction factors F_{flow} and F_{STP} for correcting eBC concentrations. F_{flow} corrects for inlet flow errors considering leakage. F_{STP} is used to adjust concentrations to STP conditions (0 °C, 1013.25 hPa).

System flow and reference					
Q_{MAAP} (slpm)	$T_{0,MAAP}$ (°C)	$p_{0,MAAP}$ (hPa)	Q (slpm)	F_{flow}	F_{STP}
7.288	0	1013.25	7.802	1.006	1

Spot size check

Table 3: Correction factor for spot sizes F_{spot} .

Nominal spot size (cm ²)	Measured spot size (cm ²)	F_{spot}
2	Well defined spot, spot size not measured	1

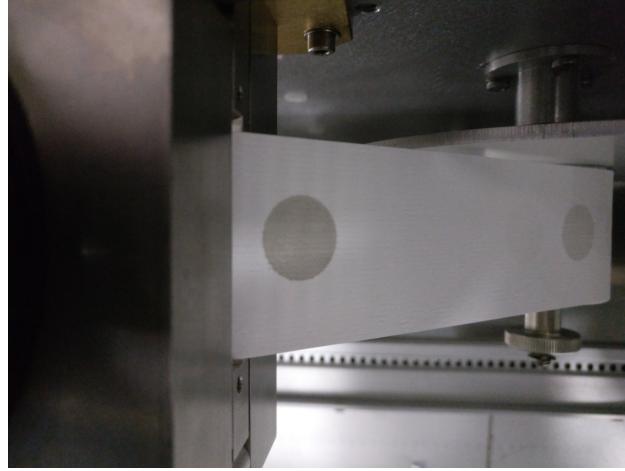


Figure 1: New spot from MAAP (159) on filter tape.

Instrumental noise

Table 4: Noise parameters measured with filtered air.

Wavelength (nm)	Data points	Median (ng/m ³)	10th perc (ng/m ³)	90th perc (ng/m ³)	Mean (ng/m ³)	Std. dev (ng/m ³)	Error of mean (ng/m ³)
660	360	2	-24	31	-1	71	4

Comparison to reference MAAP

Table 5: Correlation parameter of eBC coefficients from MAAP (159) and reference MAAP.

Wavelength (nm)	Slope	Error	R ²
660	1.039	0.01	0.997

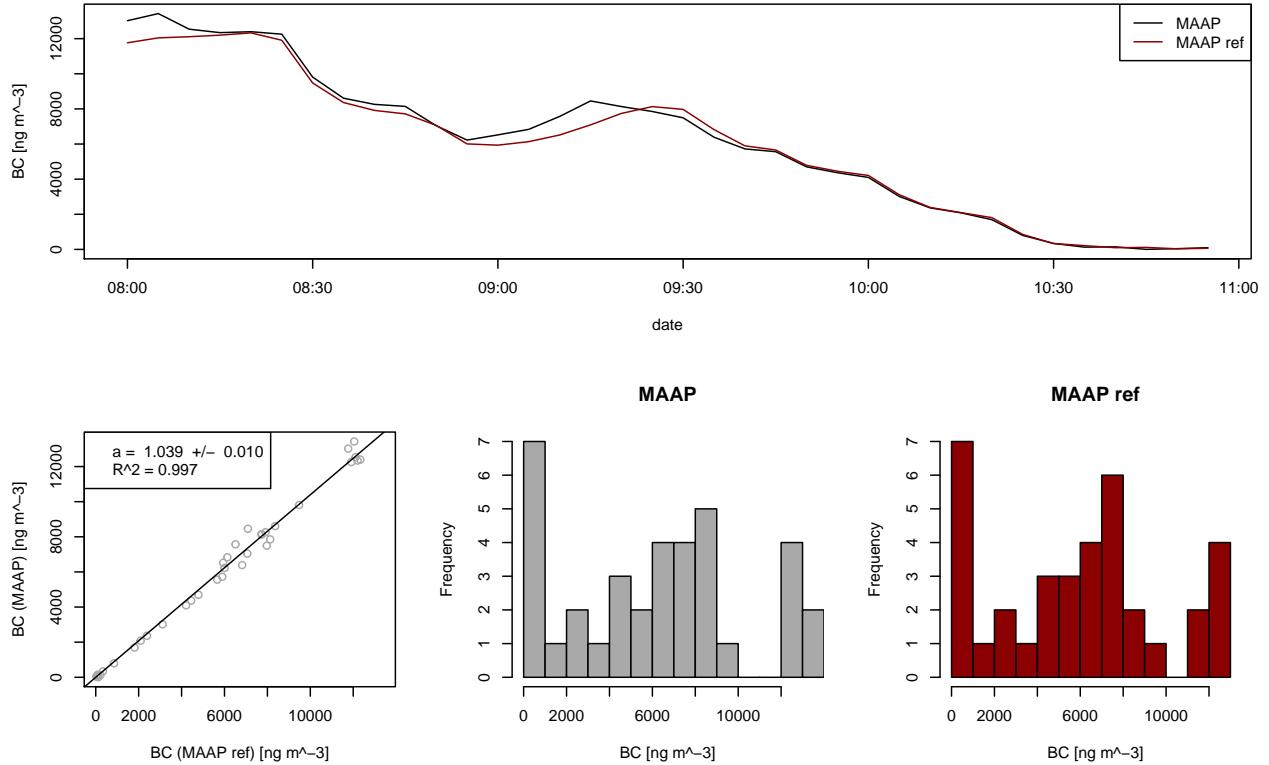


Figure 2: Correlation of eBC coefficient from MAAP (159) and reference MAAP.

Comparison to multi-wavelength absorption

Table 6: Correlation parameter of eBC coefficients from MAAP (159) and reference MAAP.

Wavelength (nm)	Slope	Error	R ²
660	1.162	0.011	0.997

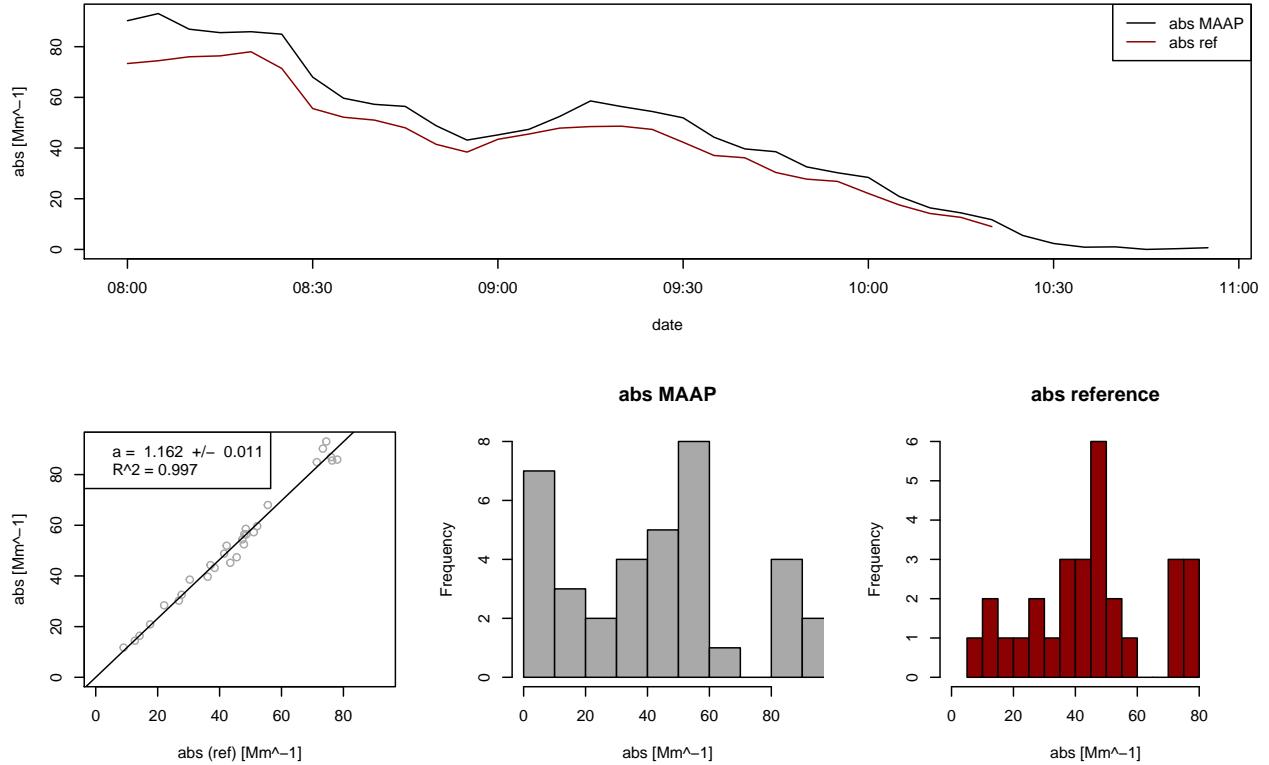


Figure 3: Correlation of absorption from MAAP (159) and the multi-wavelength absorption reference at 660 nm.