

## Intercomparison of Condensation Particle Counter

Project No.: CPC-2018-4-3

### Basic information:

**Location of the quality assurance:** TROPOS, lab: 130

**Delivery date:** -

**Setup in the laboratory:** June 6, 2018

**Comparison period:** June 6, 2018

Principal Investigator	Home Institution	Participant	Instrument
	Staatliche Betriebsgesellschaft für Umwelt und Landwirtschaft (BfUL) Altwahnsdorf 12, 01445 Radebeul Telefon: +49 351 8312-501 www.smul.sachsen.de/bful	---	DE-BFUL MPSS Dresden-Nord; TSI CPC Model 3010 # 2342

**TROPOS Reference Instrument:** Electrometer: TSI model 3068B  
# 70838596

### **Additional Equipment:**

- Bubble flow meter 'Gilibrator', Gilian (Sensidyne)

## Summary of Intercomparison:

### Pre-status:

The TSI CPC Model 3010 was in good condition.

### Final status:

The TSI CPC Model 3010 passed the quality standards of ACTRIS and GAW.

On June 6, 2018, the DE-BFUL MPSS Dresden-Nord 3010 #2342 participated in the TROPOS ACTRIS-2 CPC-Workshop.

1. Status of the wick: The wick was clean.
2. Status of the CPC: The CPC was working properly.
3. Final CPC-Workshop: The TSI CPC Model 3010 reached 98% efficiency at 40 nm. The Dp50 is at 10.1 nm. The CPC efficiency curve corresponds to the standard.

## Final status: 06.06.2018

Dp in nm	counting efficiency
40	0.98
30	0.95
20	0.90
15	0.82
13	0.71
11	0.57
10	0.47
9	0.37
8	0.23
7	0.10
6	0.02
5	0.00


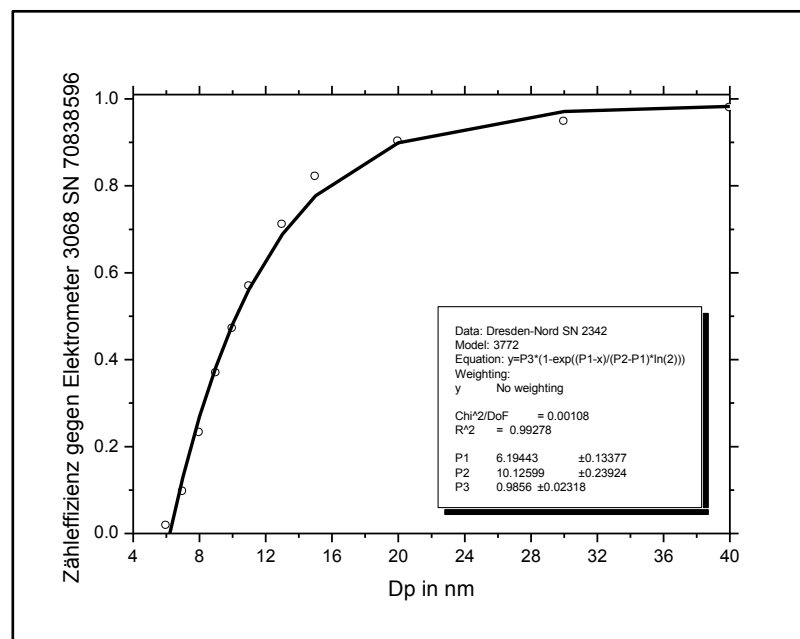


Figure 01: CPC efficiency curve based on Electrometer TSI 3068B. Serial number: 70838596



**Figure 02:** Inter-comparison of ambient air conditions between Reference CPC and CPC DDN.

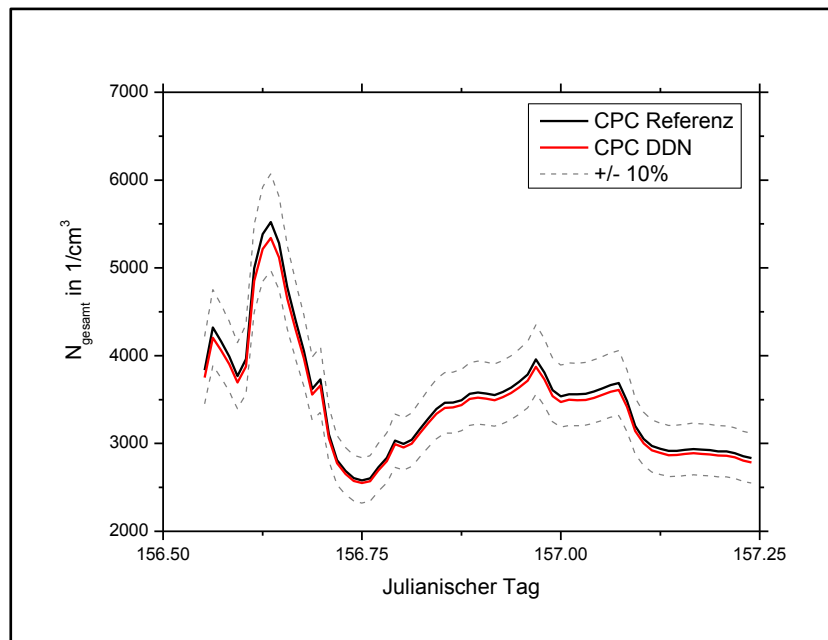

**Physikalisch-Technische Bundesanstalt  
Braunschweig und Berlin**  
Nationales Metrologieinstitut



## Kalibrierschein Calibration Certificate

Gegenstand:  
*Object:* Aerosol Elektrometer  
ID-Nummer: TSI\_3068B\_70838596

Hersteller:  
*Manufacturer:* TSI Incorporated

Typ:  
*Type:* 3068B

Kennnummer:  
*Serial No.:* 70838596

Auftraggeber:  
*Applicant:* AG 3.23 - Herr Nowak, Tel.: 3228

Anzahl der Seiten:  
*Number of pages:* 4

Geschäftszeichen:  
*Reference No.:* PTB AG 2.11-1461323527-0327

Kalibrierzeichen:  
*Calibration mark:* 20790 PTB 16

Datum der Kalibrierung:  
*Date of calibration:* 22.04.2016

Im Auftrag:  
*On behalf of PTB:* Braunschweig, 04. Mai. 2016

Im Auftrag:  
*On behalf of PTB:*

391 008 n

Dr. B. Schumacher

Siegel  
*Seal*



C. Rohrig

Kalibrierscheine ohne Unterschrift und Siegel haben keine Gültigkeit. Dieser Kalibrierschein darf nur unverändert weiterverbreitet werden. Auszüge bedürfen der Genehmigung der Physikalisch-Technischen Bundesanstalt.

*Calibration certificates without signature and seal are not valid. This calibration certificate may not be reproduced other than in full. Extracts may be taken only with permission of the Physikalisch-Technische Bundesanstalt.*