



**World Calibration Centre
for Aerosol Physics**

Leibniz-Institut für Troposphärenforschung Permoserstraße 15 04318 Leipzig



**Leibniz Institute for
Tropospheric Research**

CPC Model: TSI CPC Ref4 SN 3772142501

CPC Serial Number: 3772142501

Customer: WCCAP Reference CPC

Description: Calibration of a Condensation Particle Counter (CPC, Model TSI
CPC Ref4 SN 3772142501)

Date of Calibration: January 24, 2020

Certificate / Reference: WCCAP

Date of issue: January 24, 2020

Signature:

Reviewed by: **TROPOS**

Name: **Kay Weinhold**

Page 1 / 3

Leibniz-Institut für Troposphärenforschung e.V.
Telefon: +49 341 2717-7060
Telefax: +49 341 2717-99-7060
info@tropos.de
<http://www.tropos.de>

Commerzbank Leipzig
KTO 102 14 50
BLZ 860 400 00
IBAN: DE77 8604 0000 0102 1450 00
SWIFT CODE: COBADEFF 860

Mitglied der
The logo for Leibniz-Gemeinschaft, featuring the word 'Leibniz' in a stylized, cursive script font.
Leibniz-Gemeinschaft



World Calibration Centre
for Aerosol Physics



Leibniz Institute for
Tropospheric Research

Date of arrival of instrument in calibration lab: *January 24, 2020*
Instrument: *Condensation Particle Counter*
Model and serial number of instrument: *TSI CPC Ref4 SN 3772142501*

Result of physical inspection: *no damages*
Result of functional test: *functional test successful, no problems*

Internal parameters of instrument *nominal flow rate 1.0 l/min*

Model and identification number of aerosol electrometer: *TSI Electrometer Model 3068, S/N 70838596*

Electrometer calibration certificate: *September 5, 2018, calibrated at PTB Braunschweig*

Corrections of electrometer, for instance, differing flow rate: *Within tolerance range (+/-2%); reference: 4.0 l/min, measured: 4.000 l/min*

Software for recording: *LabView 2010; National Instruments; Program „LabCount.vi“*

Date of calibration: *January 24, 2020*
Lab temperature and pressure: *23.45°C, 1001 mbar*
Measured aerosol flow rate of CPC: *0.998 l/min*
Uncertainty in measured flow rate: *3%*
Flowmeter used: *Gilian Gilibrator V; S/N 1711008-S, January, 2018*

Particles and gases used for calibration: *silver particles and nitrogen*
Method of particle generation: *tube furnace generator*
Zero measurement of instrument: *0 particles/cm³ in 5 minutes*

Results (using pulse output):

Particle size (nm)	40	30	20	10	08
Number concentration (cm-3)	938	1288	1699	716	829
Counting efficiency η	0.97	0.96	0.95	0.69	0.47
Particle size (nm)	06				
Number concentration (cm-3)	125				
Counting efficiency η	0.07				



World Calibration Centre
for Aerosol Physics



Leibniz Institute for
Tropospheric Research

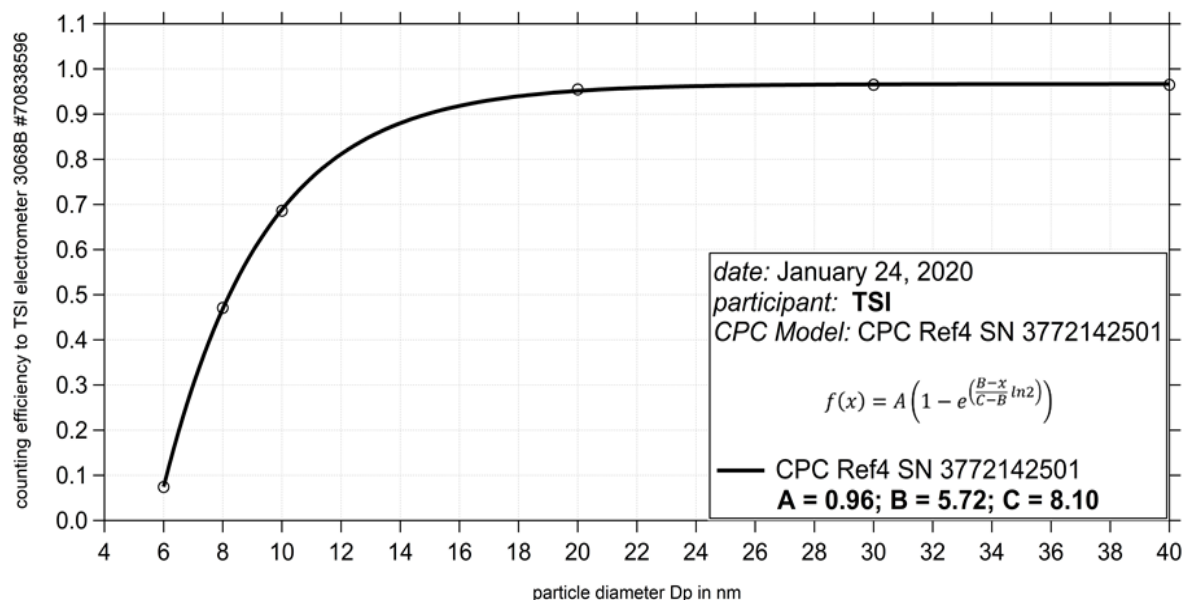


Fig. 1: Counting efficiency for TSI CPC Ref4 SN 3772142501 CPC against aerosol electrometer 3068 S/N 70838596; silver particles between 6 and 40 nm were used for calibration; the calculated Dp50 is 8.10 nm.

Status information:

Status	T SAT	T CON	T OPT	T CAB	P AMB	P VAC
from display	39.0	22.0	40.0	32.1	100.0	
Status	P OR	P NO	Laser	LV	flow	P INLET
from display	79.5	2.7	59	full	0.998	

Date of issue: January 24, 2020

Reference: TSI electrometer, model 3068, SN 70838596

Reviewed: TROPOS / Kay Weinhold