



**World Calibration Centre  
for Aerosol Physics**

Leibniz-Institut für Troposphärenforschung Permoserstraße 15 04318 Leipzig



**Leibniz Institute for  
Tropospheric Research**

**CPC Model:** TSI CPC 3772

**CPC Serial Number:** 3772142501

**Customer:** TROPOS

**Description:** Calibration of a Condensation Particle Counter (CPC, Model 3772)

**Date of Calibration:** 08 05, 2020

**Summary of Intercomparison:**

The candidate passed the quality standards of ACTRIS and GAW. The candidate reached 98% efficiency at 40 nm. The Dp50 is at 7.93 nm. The CPC efficiency curve corresponds to the standard of ACTRIS and GAW.

Certificate / Reference: WCCAP

Date of issue: May 17, 2020 Signature:

Reviewed by: **TROPOS**

Name: **Kay Weinhold**

Page 1 / 3



World Calibration Centre  
for Aerosol Physics



Leibniz Institute for  
Tropospheric Research

**Date of arrival of instrument in calibration lab:** -  
**Instrument:** *Condensation Particle Counter*  
**Model and serial number of instrument:** *CPC 3772 S/N 3772142501*

**Result of physical inspection:** *no damages*  
**Result of functional test:** *functional test successful, no problems*

**Internal parameters of instrument** *nominal flow rate 1.0 l/min*

**Model and identification number of aerosol electrometer:** *TSI Electrometer Model 3068, S/N 70838596*

**Electrometer calibration certificate:** *September 5, 2018, calibrated at PTB Braunschweig*

**Corrections of electrometer, for instance, differing flow rate:** *Within tolerance range (+/-2%); reference: 4.0 l/min, measured: 4.000 l/min*

**Software for recording:** *LabView 2010; National Instruments; Program „LabCount.vi“*

**Date of calibration:** *May 08, 2020*  
**Lab temperature and pressure:** *23.0°C, 999 mbar*  
**Measured aerosol flow rate of CPC:** *0.997 l/min*  
**Uncertainty in measured flow rate:** *3%*  
**Flowmeter used:** *Gilian Gilibrator V; S/N 1711008-S, January, 2018*

**Particles and gases used for calibration:** *silver particles and nitrogen*  
**Method of particle generation:** *tube furnace generator*  
**Zero measurement of instrument:** *0 particles/cm<sup>3</sup> in 5 minutes*

**Results (using pulse output):**

Particle size (nm)	40	30	20	15	10
Number concentration (cm-3)	980	1352	1138	1339	1290
Counting efficiency $\eta$	0.98	0.98	0.98	0.93	0.73
Particle size (nm)	09	08	07	06	05
Number concentration (cm-3)	1122	590	358	89	0
Counting efficiency $\eta$	0.64	0.50	0.31	0.07	0.00



World Calibration Centre  
for Aerosol Physics



Leibniz Institute for  
Tropospheric Research

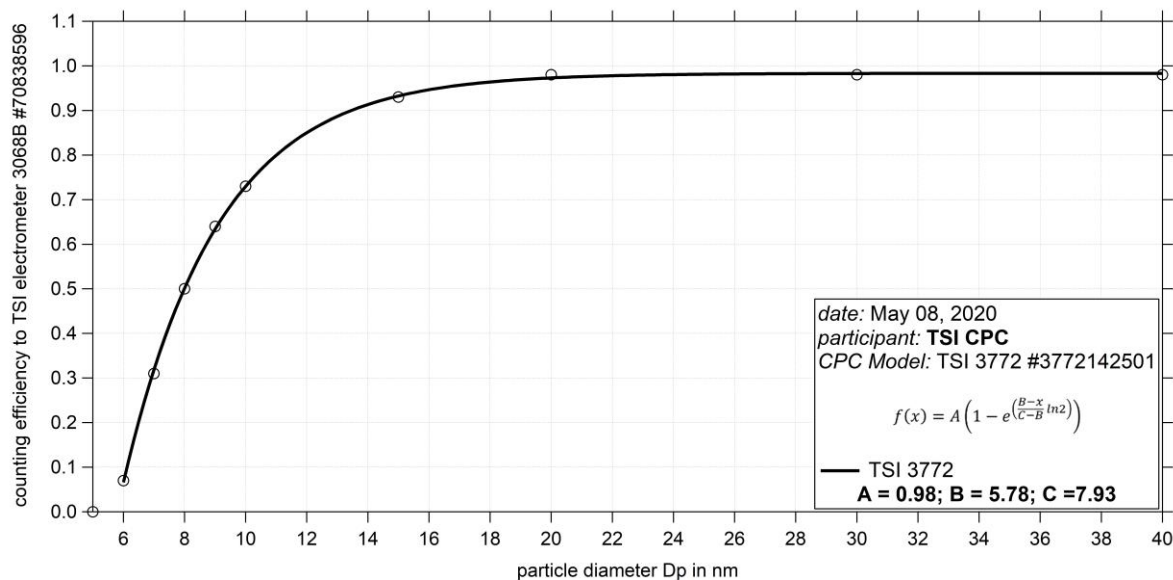


Fig. 1: Counting efficiency for CPC 3772S/N 3772142501 against aerosol electrometer 3068 S/N 70838596; silver particles between 5 and 40 nm were used for calibration; the calculated Dp50 is 7.93 nm.

**Status information:**

Status	T SAT	T CON	T OPT	T CAB	P AMB	P VAC
from display	39.0	22	40.0	30.0	99.8	-
Status	P OR	P NO	Laser	LV	flow	P INLET
from display	81.7	2.5	52	full	0.997	-

**Date of issue:** May 18, 2020

Reference: TSI electrometer, model 3068, SN 70838596

Reviewed: TROPOS / Kay Weinhold