



World Calibration Centre
for Aerosol Physics

Leibniz-Institut für Troposphärenforschung, Permoserstraße 15, 04318 Leipzig



Leibniz Institute for
Tropospheric Research

CPC Model: TSI CPC 3772

CPC Serial Number: 70711210

Customer: DWD Hohenpeißenberg

Description: Calibration of a Condensation Particle Counter (CPC, Model 3772)

Date of Calibration: October 27, 2020

Summary of Intercomparison:

The candidate passed the quality standards of ACTRIS and GAW. The candidate reached 100% efficiency at 40 nm. The Dp_{50} is at 7.68 nm. The CPC efficiency curve corresponds to the standard of ACTRIS and GAW.

Certificate / Reference: WCCAP

Date of issue: October 27, 2020

Signature:

Reviewed by: **TROPOS**

Name: **Kay Weinhold**

Page 1 / 4



World Calibration Centre
for Aerosol Physics



Leibniz Institute for
Tropospheric Research

Date of arrival of instrument in calibration lab:	<i>October 23, 2020</i>
Instrument:	<i>Condensation Particle Counter</i>
Model and serial number of instrument:	<i>CPC 3772 SN 70711210</i>
Result of physical inspection:	<i>no damages</i>
Result of functional test:	<i>functional test successful, no problems</i>
Internal parameters of instrument	<i>nominal flow rate 1.0 l/min</i>
Model and identification number of aerosol electrometer:	<i>TSI Electrometer Model 3068, SN 70838596</i>
Electrometer calibration certificate:	<i>September 5, 2018, calibrated at PTB Braunschweig</i>
Corrections of electrometer, for instance, differing flow rate:	<i>Within tolerance range (+/-2%); reference: 4.0 l/min, measured: 4.000 l/min</i>
Software for recording:	<i>LabView 2010; National Instruments; Program „LabCount.vi“</i>
Date of calibration:	<i>October 27, 2020</i>
Lab temperature and pressure:	<i>23.0°C, 988 mbar</i>
Measured aerosol flow rate of CPC:	<i>0.990 l/min</i>
Uncertainty in measured flow rate:	<i>3%</i>
Flowmeter used:	<i>Gilian Gilibrator V; SN 1711008-S, January, 2018</i>
Particles and gases used for calibration:	<i>silver particles and nitrogen</i>
Method of particle generation:	<i>tube furnace generator</i>
Zero measurement of instrument:	<i>0 particles/cm³ in 10 minutes</i>



World Calibration Centre
for Aerosol Physics



Leibniz Institute for
Tropospheric Research

	Unit	Status
Model	-	TSI 3772
SN	-	70711210
Firmware	-	2.9
Date	-	-
TSI Software Version	-	-
Saturator Temperature	°C	39.00
Condenser Temperature	°C	22.00
Optics Temperature	°C	40.00
Cabinet Temperature	°C	29.00
Ambient Pressure	kPa	98.90
Vacuum Pressure	kPa	-
Inlet Pressure	kPa	-
Critical Orifice Pressure	kPa	82.70
Aerosol Nozzle Pressure	kPa	2.70
Laser Current	mA	53.00
Liquid Level	-	full
Aerosol Flow	l/min	0.99
Zero	avg 10 min	0

Diameter	EL 3068B (#/cm ³)	BNC (pulse output)	
		Concentration (#/cm ³)	Efficiency (μ)
40	1054	1060	1.01
40	1273	1285	1.01
30	1085	1092	1.01
20	1008	1032	1.02
15	1187	1171	0.99
14	-	-	-
12	983	901	0.92
11	-	-	-
10	1765	1414	0.80
9	1045	751	0.72
8	1331	760	0.57
7	1170	401	0.34
6	1257	57	0.05
5	1030	0	0.00



World Calibration Centre
for Aerosol Physics



Leibniz Institute for
Tropospheric Research

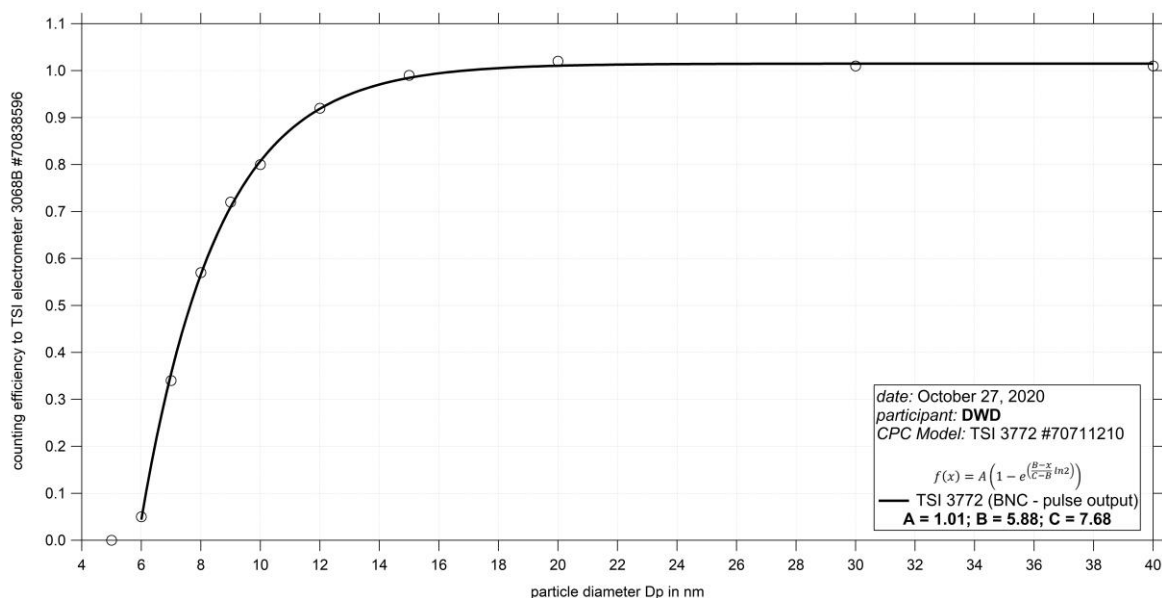


Fig. 1: Counting efficiency for TSI-CPC 3772 SN 70838335 against aerosol electrometer 3068 SN 70838596; silver particles between 5 nm and 40 nm were used for calibration; the calculated D_{p50} from the BNC (pulse output) is 7.68 nm.

Date of issue: October 27, 2020

Reference: TSI electrometer, model 3068, SN 70838596

Reviewed: TROPOS / Kay Weinhold