

## Intercomparison of Mobility Particle Size Spectrometers

*Project No.:* *MPSS-2020-3-16*

*Principal Investigator:* *JP Dr. Anke C. Nölscher*

*Home Institution:* *Universität Bayreuth*

*Participant:* -


*Candidate:* MPSS Bayreuth  
*Made by:* TROPOS  
*Counter (SN):* TSI CPC 3772

*Location of the quality assurance:* TROPOS Leipzig, lab 118

*Comparison period:* July 02, 2020 – July 03, 2020

*Last Intercomparison (with Project No.):* -


**PSL Scan: Latex 203 nm +/- 4 nm**

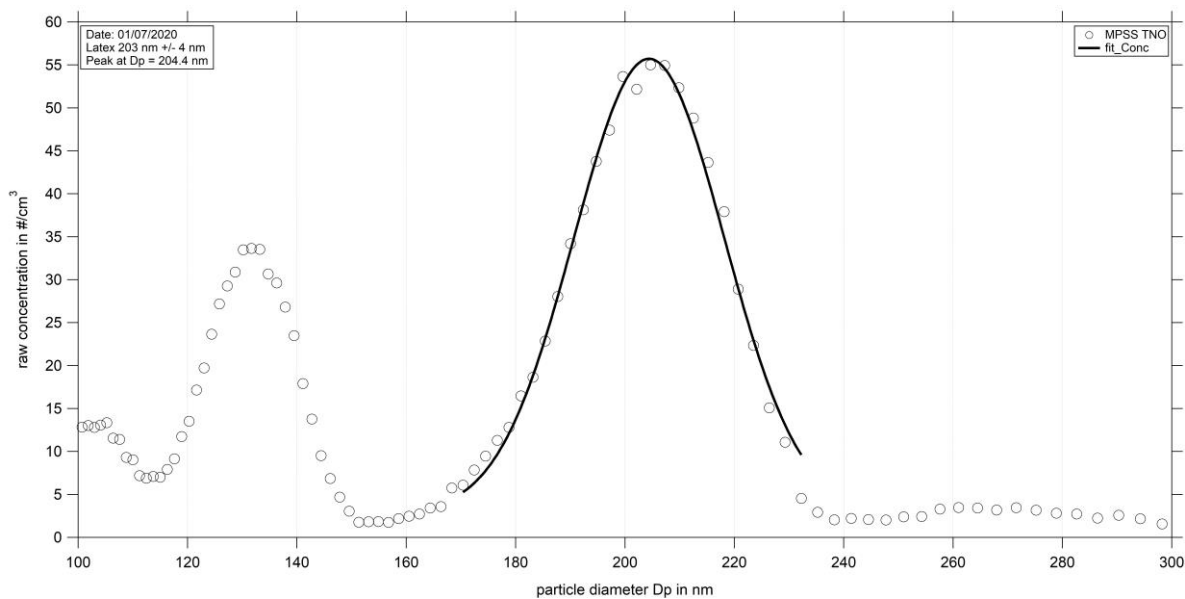


**Figure 01:** Measurement of latex 203 nm – MPSS Bayreuth: Particle size distribution of latex 203 nm on July 01<sup>th</sup>, 2020. The peak shows at 204.4nm.

**Intercomparison between TROPOS Reference Instrument No. 1 and MPSS Bayreuth**


**02.07.2020 06:00 PM – 03.07.2020 06:00 AM**

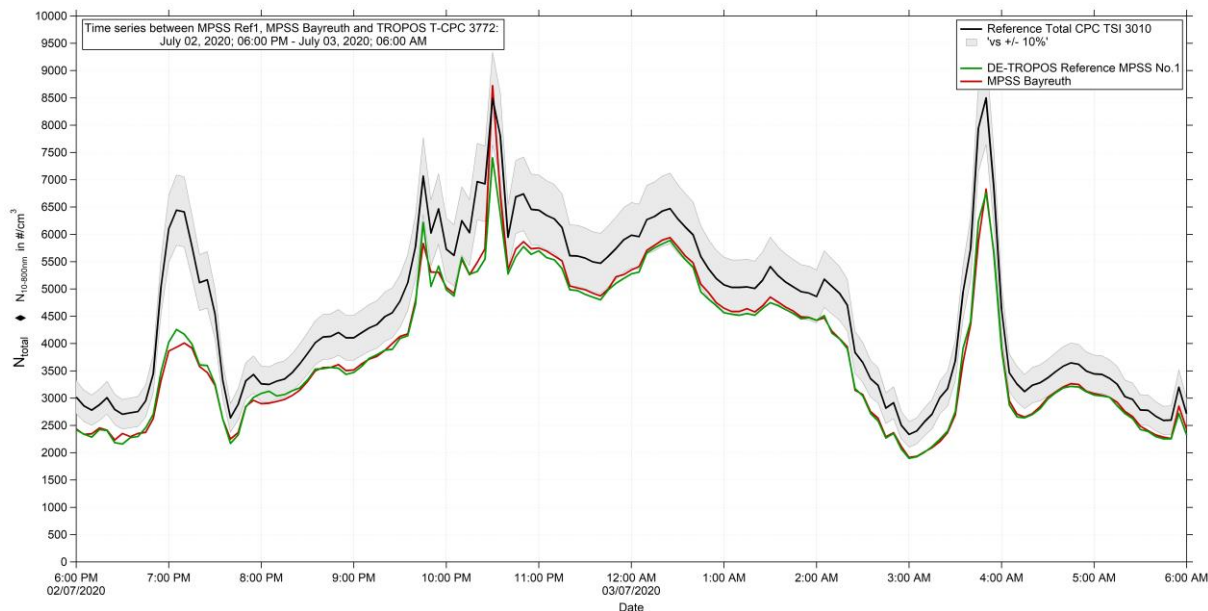


**Figure 02:** Time series (July 02, 2020 6 PM – July 03, 2020 6 AM) of the integrated particle number concentration (N<sub>10-800nm</sub>) of the MPSS and total number concentration (N<sub>total</sub>) of the Reference TSI-CPC Model 3772. Multiple charge correction, internal diffusion losses, CPC flow corrections.

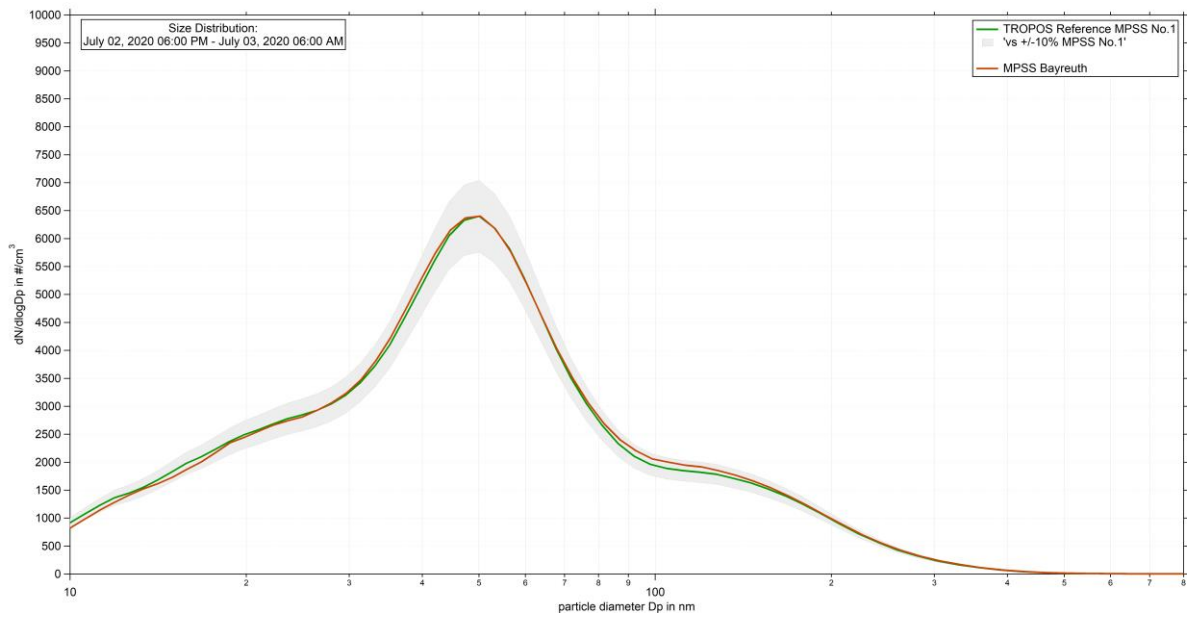

**Figure 03:** Particle size distribution for TROPOS Reference MPSS No.1 and MPSS Bayreuth, flow corrections, multiple charge correction and diffusion loss corrections are included.

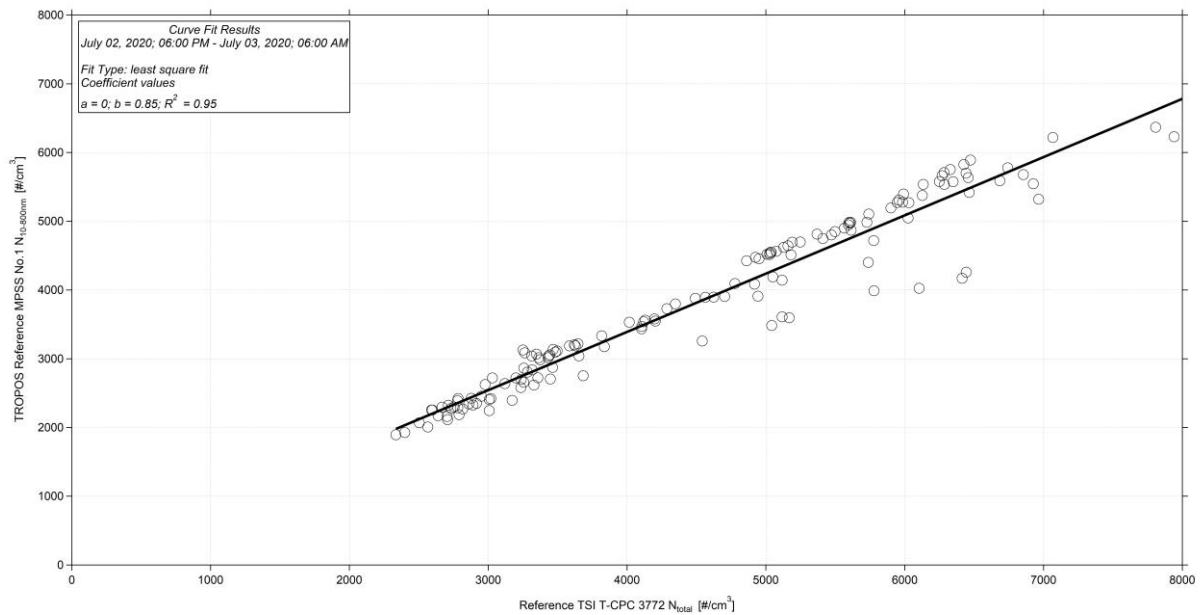

**Figure 04:** Linear regression between DE-TROPOS Reference T-CPC Model 3772 and DE-TROPOS Reference MPSS No.1.

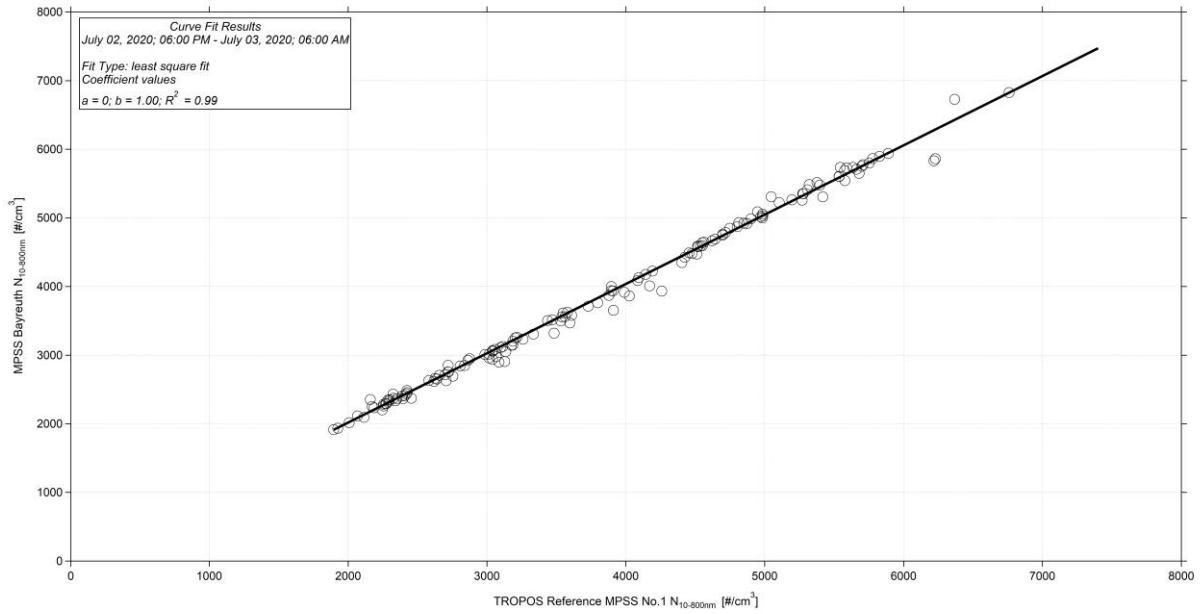

**Figure 05:** Linear regression between DE-TROPOS Reference MPSS No.1 and MPSS Bayreuth.